

# Application News

## No. L528

### High Performance Liquid Chromatography

## Measuring Hexavalent Chromium Compounds in Atmospheric Dust

### - Ion Chromatography Post-Column Absorption Spectroscopy Method -

In March 2018, Japan's Ministry of the Environment issued the "Manual of measurement methods for hazardous air pollutants - Measurement method for hexavalent chromium compounds in atmospheric dust" (in Japanese). In this manual, hexavalent chromium compounds are measured using the alkali-impregnated filter collection - ion chromatography post-column derivatization spectroscopic absorption method. Diphenyl carbonohydrazide, which specifically reacts with hexavalent chromium, is used as the post column derivatization reagent. The concentration of hexavalent chromium that can be measured by this method is 0.069 to 3.47 ng/m<sup>3</sup>, in terms of concentrations in atmospheric dust. This article introduces an example measurement using the Prominence™ HPLC.

A. Ieuji

#### Overview of the Measurement Method


An alkali-impregnated cellulose filter is first prepared by using sodium bicarbonate solution. Air is passed through this filter at a flow rate of 5 L/min for 24 hours. The material collected on the filter is eluted with ultra-pure water and used as the measurement sample.

The hexavalent chromium ions in the sample solution are separated using an anion exchange column. Then, following post-column derivatization using a diphenyl carbonohydrazide/sulfate solution, absorbance at the wavelengths between 520 to 540 nm are to be measured.

Diphenyl carbonohydrazide, which is the reaction reagent, contacts hexavalent chromium ions and turns into diphenylcarbazone and then forms a diphenylcarbazide-chromium complex.

The measurement system requires plastic components for all liquid contact sections from the reaction reagent delivery pump and after, including the detector, since the reagent contains 0.5 mol/L sulfate. In addition, the detector light source must be a tungsten (W) lamp, which is suited for the wavelengths to be detected.


Fig. 1 shows the flow line diagram of the post-column system and Table 1 lists the measurement conditions.

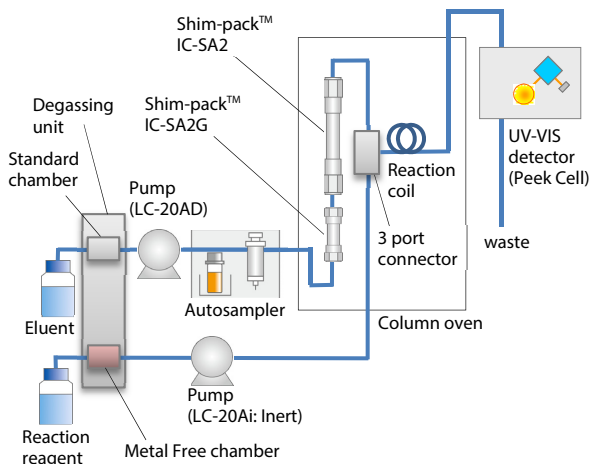

**Fig. 1 Hexavalent Chromium Measurement System Flow Line Diagram**

**Table 1 Measurement Conditions**


■ Separation	
Column	: Shim-pack™ IC-SA2 (250 mm L., 4.0 mm I.D.)
Guard column	: Shim-pack™ IC-SA2G (10 mm L., 4.6 mm I.D.)
Eluent	: 10 mmol/L Sodium Carbonate/ 10 mmol/L Sodium Bicarbonate
Flow rate	: 1.0 mL/min
Column temp.	: 40 °C
■ Injection vol.	: 0.25 mL
■ Post Column Derivatization	
Reaction reagent	: 2 mmol/L Diphenyl carbonohydrazide - 10 %-Methanol-0.5 mol/L Sulfate
Flow rate	: 0.2 mL/min
Reaction temp.	: 40 °C
Reaction coil	: 0.5 mm I.D.×8 m L. (PTFE)
■ Detection	: UV-VIS detector at 540 nm (SPD-20AV, W lamp, Inert Cell)

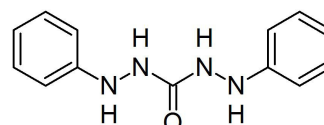

**Fig. 2 Diphenyl Carbonohydrazide**

#### Measurement of Standard Sample Solutions

Fig. 3 shows the chromatograms of potassium dichromate (JIS K8005) standard solutions diluted to between 0.1 and 5.0 ng/mL using ultra-pure water.

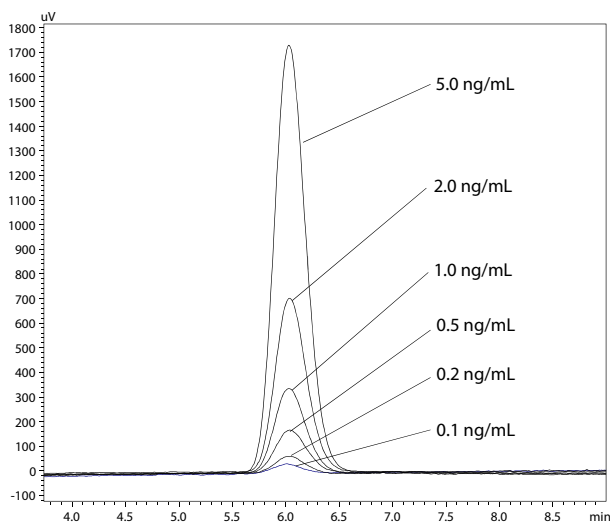

**Fig. 3 Chromatograms of Standard Solutions**

### Linearity of Calibration Curve

Fig. 4 shows the calibration curve created using sample solutions of differing concentrations as shown in Fig. 3.

Linearity in the range from 0.1 to 5.0 ng/mL was favorable at above  $r^2 = 0.999$ .

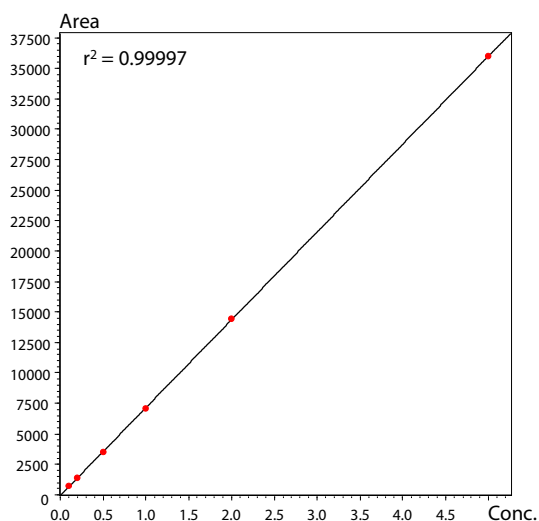


Fig. 4 Linearity of Calibration Curve

### Repeatability of the Standard Solutions

Fig. 5 shows the chromatograms obtained by measuring the 0.1 ng/mL standard solution five times repeatedly. Table 2 lists the peak area, quantitation value (concentration) based on the calibration curve shown in Fig. 4, and the accuracy of each measurement.

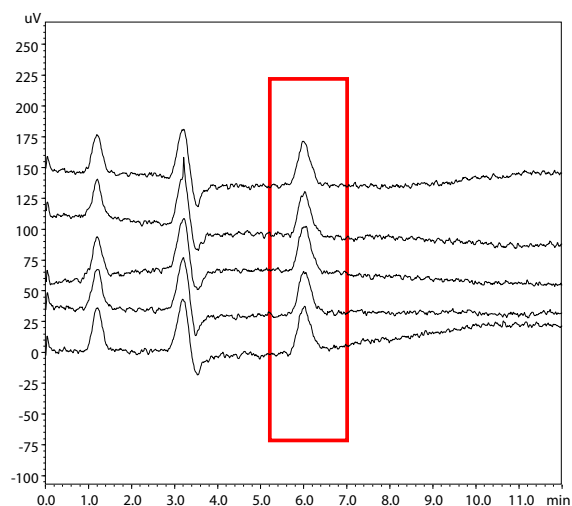


Fig. 5 Chromatograms from Repeated Measurements of 0.1 ng/mL Standard Solution

Table 2 Results from Repeated Measurements of 0.1 ng/mL Standard Solution

Measurement	Area	Concentration (ng/mL)	Accuracy (%)
1	724	0.099	99.1
2	719	0.098	98.5
3	743	0.102	101.7
4	731	0.100	100.0
5	736	0.101	100.8
Average	731	0.100	
%RSD	1.3	1.6	

### Influence of Sample Matrix

Fig. 6 compares the chromatograms of the standard solution when diluted, respectively, with water and with sodium bicarbonate solution, which is used to prepare the alkali-impregnated filter. Sodium carbonate released from the alkali-impregnated filter is a matrix and the elution strength becomes slightly stronger, causing a change in the elution time by a few seconds. However, we can see that the peak shapes are the same. The chromatograms are shown in (a) before retention time alignment and in (b) after retention time alignment to compare the peak shapes.

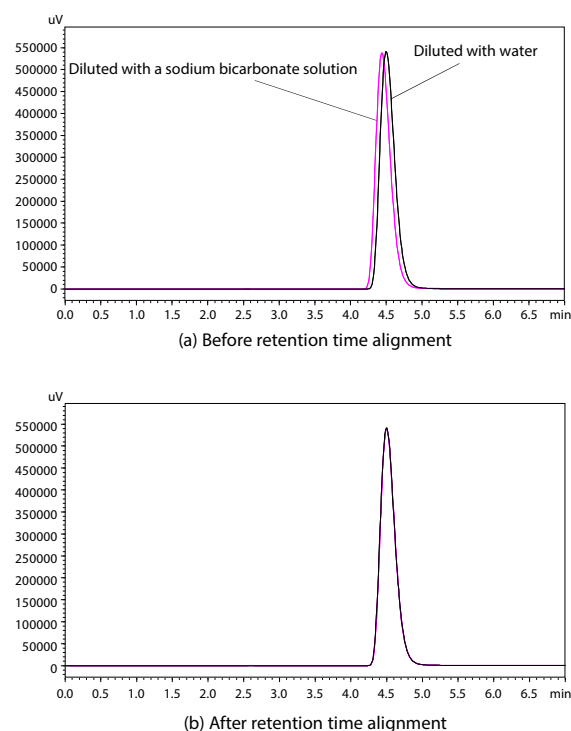


Fig. 6 Comparison of Dilution Solvents with a 1000 ng/mL Standard Solution

Prominence and Shim-pack are trademarks of Shimadzu Corporation.

First Edition: Nov. 2018



For Research Use Only. Not for use in diagnostic procedure.

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. Shimadzu disclaims any proprietary interest in trademarks and trade names used in this publication other than its own. See <http://www.shimadzu.com/about/trademarks/index.html> for details.

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change without notice.

Shimadzu Corporation

[www.shimadzu.com/an/](http://www.shimadzu.com/an/)